


PAVE#	PAVE DESCRIPTION	ITEM 3	ITEM 3 DESCRIPTION
0904KT	PTN12-SS-200-9P-KT20-24-48	KT20	CABLE T/C TYPE K 20AWG TEFLON (YEL/RED)
0904TT	PTN12-SS-200-9P-TT20-24-48	TT20	CABLE T/C TYPE T #20 TEFLON FEP (BLU/RED)
0904JT	PTN12-SS-200-9P-JT20-24-48	JT20	CABLE T/C TYPE J 20AWG TEFLON (WHT/RED)
0904ET	PTN12-SS-200-9P-ET20-24-48	ET20	CABLE T/C TYPE E 20AWG TEFLON (PUR/RED)

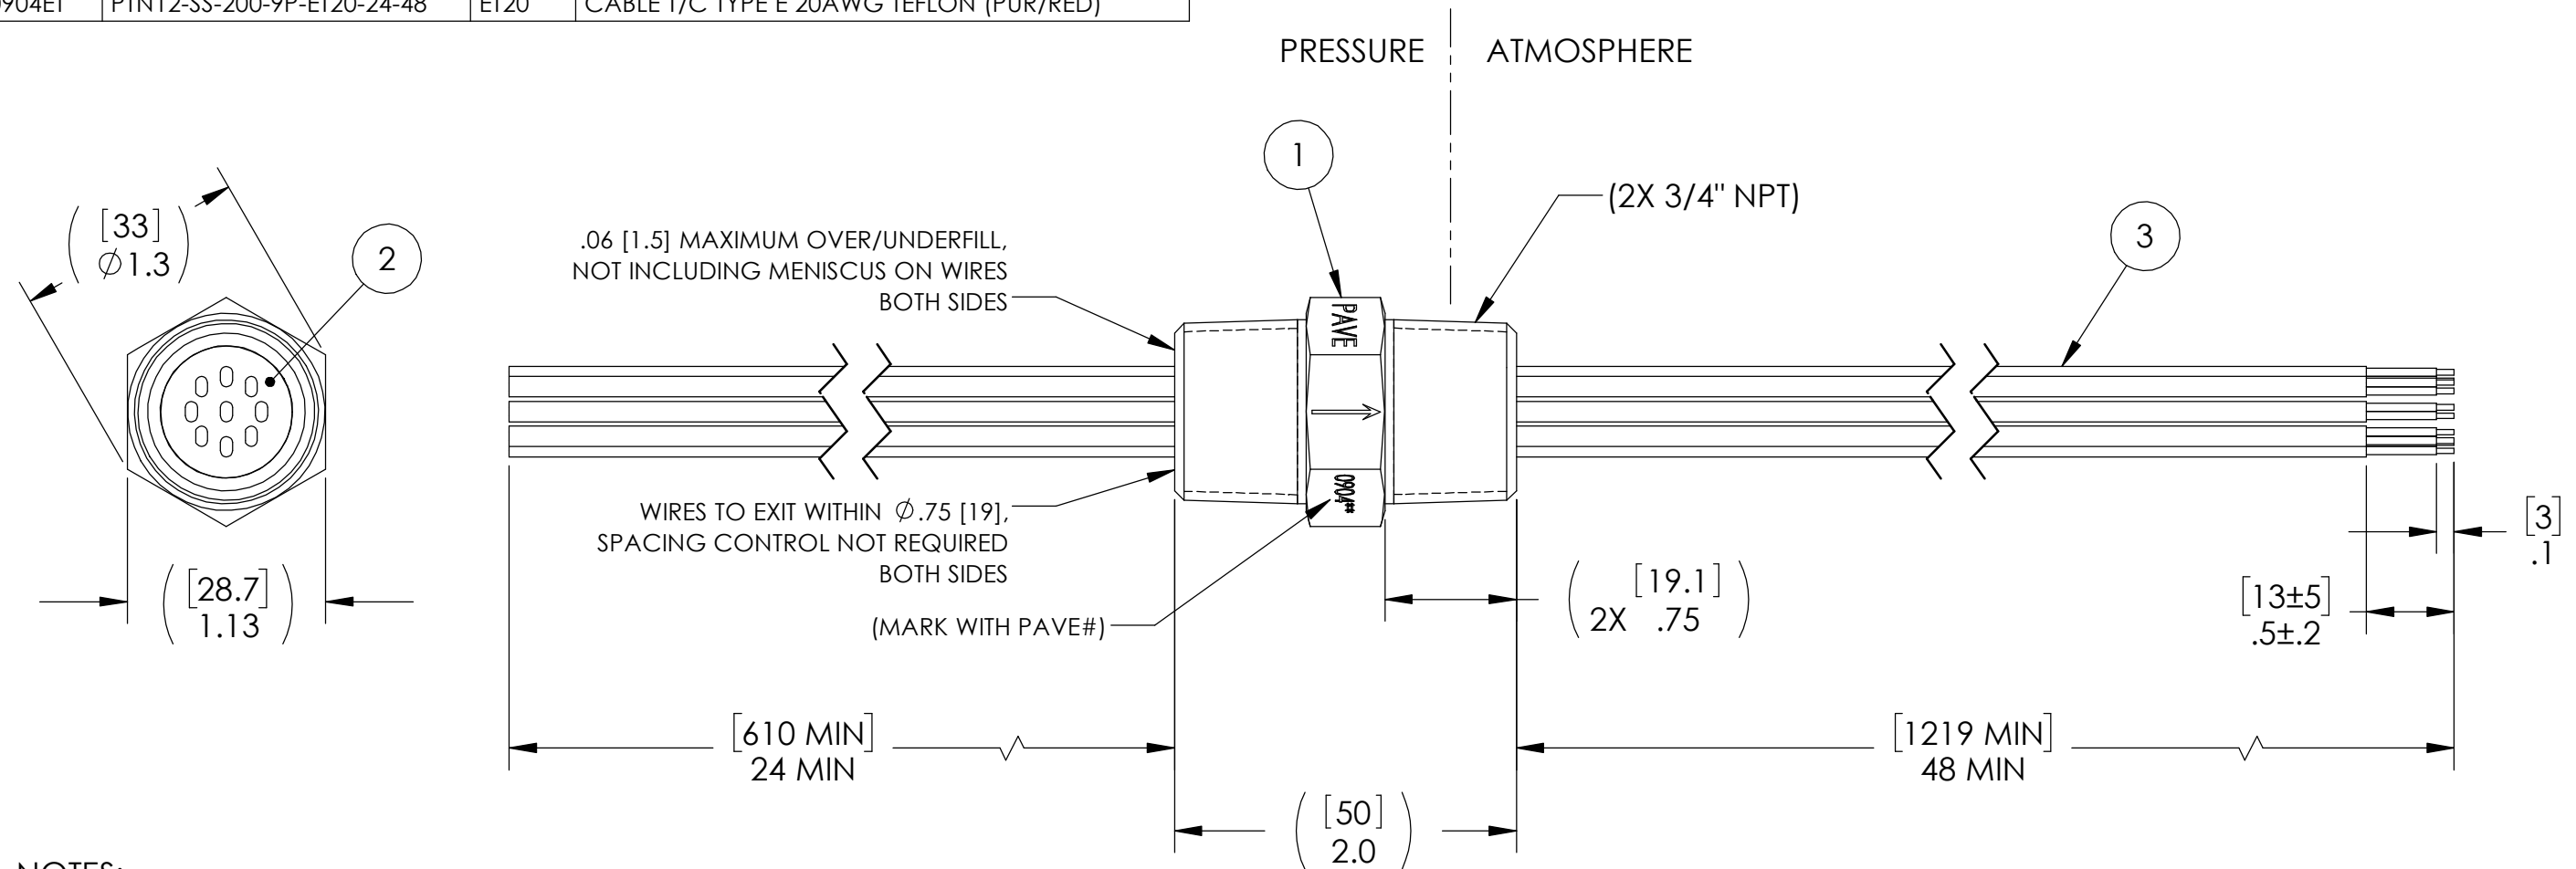

NOTES:

1. LEAK TEST: 80 PSI, NO BUBBLES 2 MINUTES MINIMUM. A GREEN PAINT DOT INDICATES THE PART HAS PASSED THE TEST.
2. HYPOT 630 VDC 500 MEGOHMS MINIMUM 0.01 SECOND MINIMUM WIRE TO WIRE AND HOUSING.
3. ALL TESTS ARE PERFORMED AT ROOM TEMPERATURE.
4. ALL PARTS MUST PASS ALL TESTS.
5. WIRE POSITIONING IS APPROXIMATE & VARIABLE.
6. COSMETIC SURFACE VOIDS SMALLER THAN $\phi 0.035$ [0.89] ARE ACCEPTABLE.
7. REF-OPERATING TEMPERATURE -20°C TO 150°C .
8. DIMENSIONS ARE INCHES [millimeters].
9. PAVE-SEAL CAN BE A BI-DIRECTIONAL HERMETIC SEAL FOR VACUUM AND MOST PRESSURES. FOR PRESSURES ABOVE 150 PSI (10 BAR), CHECK WITH SALES ENGINEERING.

3	9	SEE TABLE	SEE TABLE
2	A/R	PAVE-Seal 200	EPOXY BLACK
1	1	0073	HOUSING PTN12-SS
ITEM	QTY	PART NUMBER	DESCRIPTION

PAVE technology co.
 2751 Thunderhawk Court
 Dayton, OH 45414-3445
 U.S.A.
 tel (937) 890-1100
 fax (937) 8905165
 www.pavetechnologyco.com

DESCRIPTION
SEE TABLE

PART NUMBER **SEE TABLE MATERIAL NOTED

0904** REVISION LEVEL B PROJECTION

ALL DIMENSIONS AND TOLERANCES APPLY TO FINISHED PART IN INCHES.
 ALLOWABLE TOLERANCES UNLESS SPECIFIED OTHERWISE: NONE ± 0.5
 X.X DECIMAL ± 0.1 X.XX DECIMAL ± 0.02 X.XXX DECIMAL ± 0.005
 ANGLES ± 1 DEGREE SURFACE FINISH 128 microinch RMS