


PAVE#	ITEM 3	ITEM 3 DESCRIPTION	X	Y	PAVE DESCRIPTION
3667	KT24	CABLE T/C TYPE K 24AWG TEFLON	36 [914]	18 [457]	CF275-SS-150-36P-KT24-36-18
3667-1	KT24	CABLE T/C TYPE K 24AWG TEFLON	18 [457]	72 [1829]	CF275-SS-150-36P-KT24-18-72
3667-T	TT24	CABLE T/C TYPE T 24AWG TEFLON	36 [914]	18 [457]	CF275-SS-150-36P-TT24-36-18

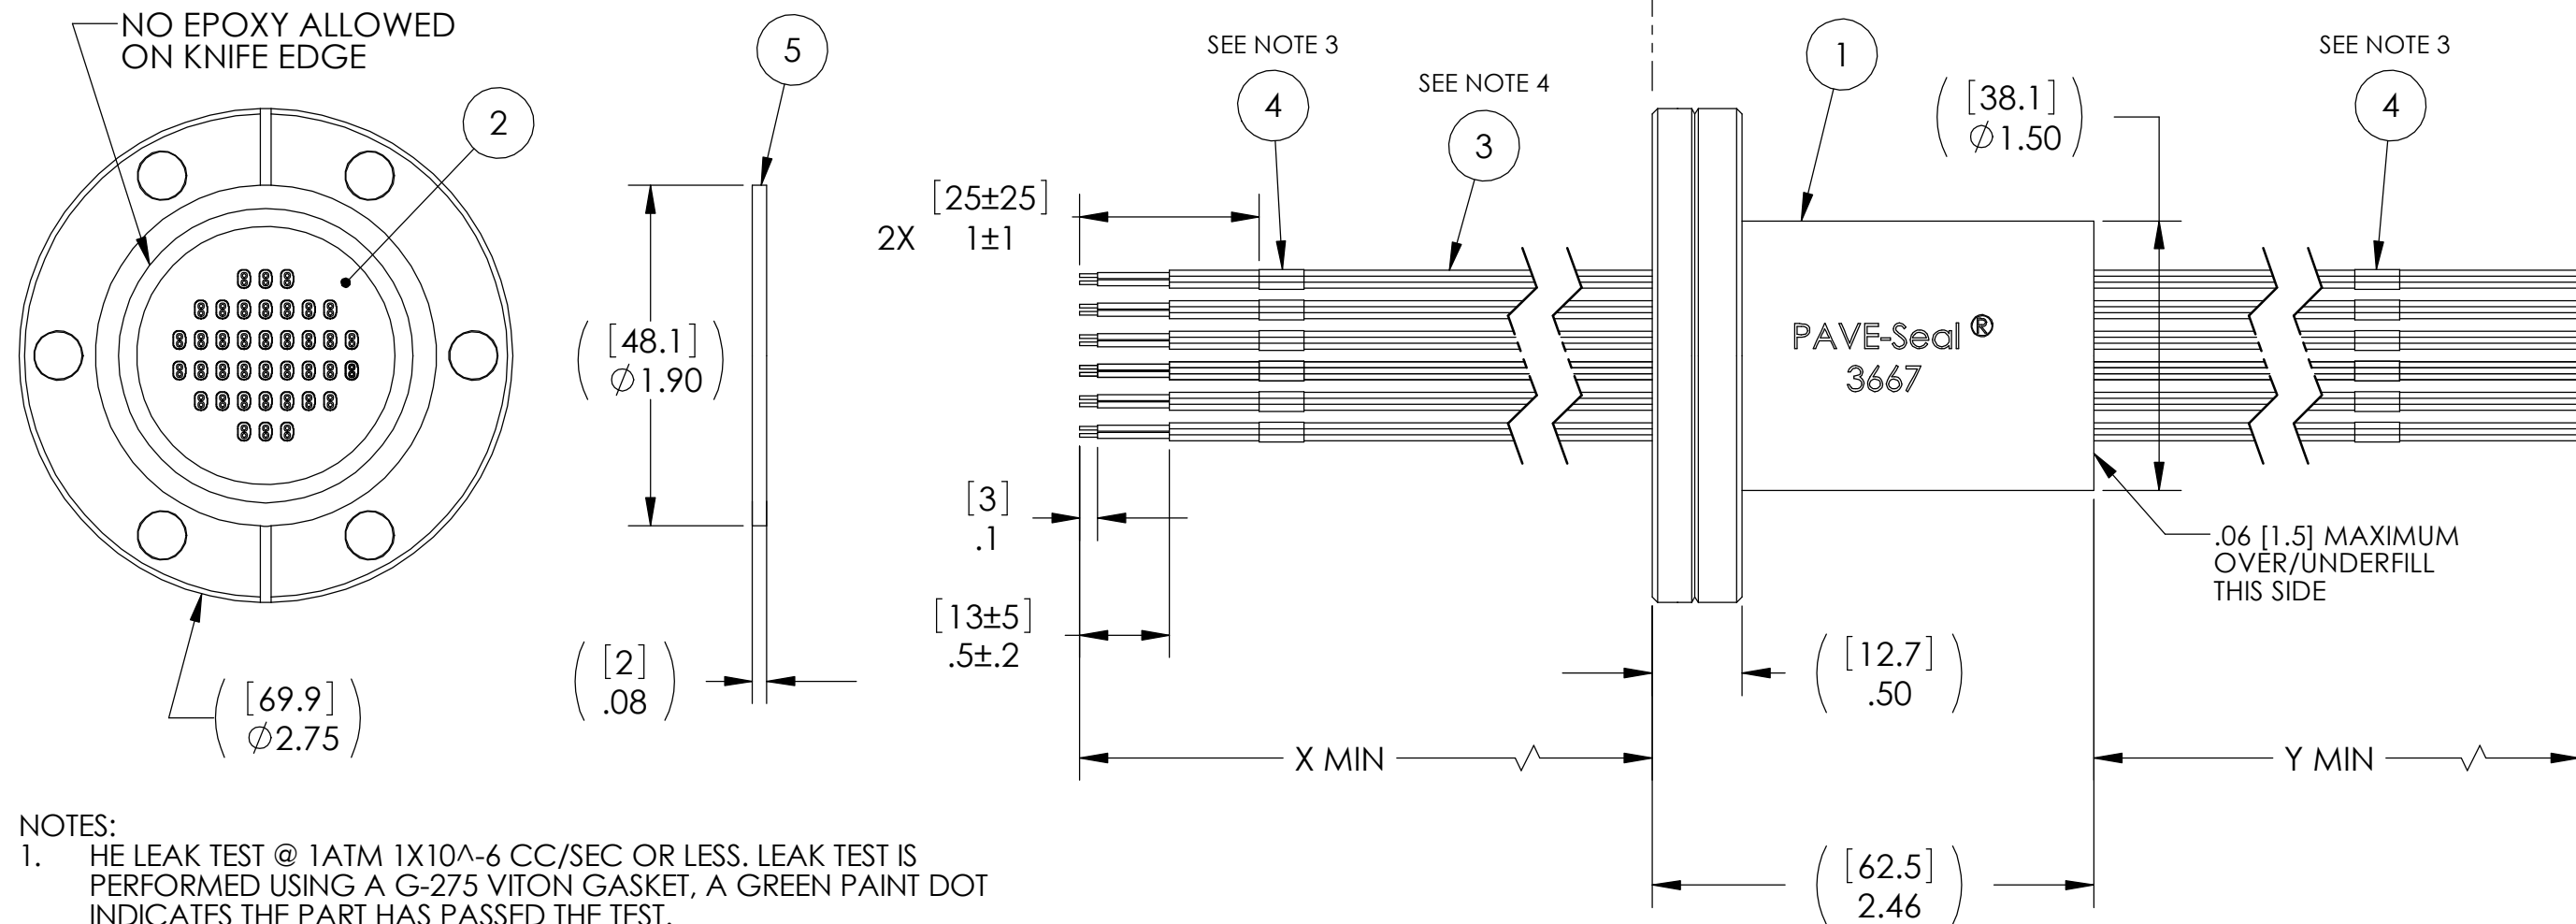

NOTES:

1. HE LEAK TEST @ 1ATM 1X10⁻⁶ CC/SEC OR LESS. LEAK TEST IS PERFORMED USING A G-275 VITON GASKET, A GREEN PAINT DOT INDICATES THE PART HAS PASSED THE TEST.
2. HYPOT 630 VDC 500 MEGOHMS MINIMUM 0.01 SECOND MINIMUM WIRE TO WIRE AND HOUSING.
3. BOTH SIDES OF ITEM 3 WILL BE MARKED WITH CORRESPONDING NUMBERS OR LETTERS.
4. MINIMUM QUANTITY 36 OF ITEM 3 REQUIRED.
5. ALL TESTS ARE PERFORMED AT ROOM TEMPERATURE.
6. ALL PARTS MUST PASS ALL TESTS.
7. WIRE POSITIONING IS APPROXIMATE & VARIABLE.
8. COSMETIC SURFACE VOIDS NOT ON O-RING SEALING SURFACES ARE ACCEPTABLE BASED ON THE SEAL'S DIAMETER:
 <= .5 [12.7] SEAL DIAMETER: ϕ .035 [.89] MAX ALLOWED VOID SIZE
 > .5 [12.7] SEAL DIAMETER: ϕ .060 [1.5] MAX ALLOWED VOID SIZE
9. DIMENSIONS ARE INCHES [millimeters].
10. REF-OPERATING TEMPERATURE RANGE -20 °C TO 125 °C.
11. PAVE-SEAL CAN BE A BI-DIRECTIONAL HERMETIC SEAL FOR VACUUM AND MOST PRESSURES. FOR PRESSURES ABOVE 150 PSI (10 BAR), CHECK WITH SALES ENGINEERING.

5	1	GASKET G-275 C	GASKET COPPER
4	A/R	-	BRADY WIRE MARKERS
3	38	SEE TABLE	SEE TABLE
2	A/R	PAVE-Seal 150	EPOXY BLACK
1	1	1473	HOUSING CF275-SS
ITEM	QTY	PART NUMBER	DESCRIPTION

PAVE technology co.

2751 Thunderhawk Court
Dayton, OH 45414-3445
U.S.A.
tel (937) 890-1100
fax (937) 8905165
www.pavetechnologyco.com

DESCRIPTION	SEE TABLE		
PART NUMBER *SEE TABLE	MATERIAL	NOTED	
3667*	REVISION LEVEL	C	PROJECTION

ALL DIMENSIONS AND TOLERANCES APPLY TO FINISHED PART IN INCHES.
 ALLOWABLE TOLERANCES UNLESS SPECIFIED OTHERWISE: NONE ±0.5
 X.X DECIMAL ±0.1 X.XX DECIMAL ±0.02 X.XXX DECIMAL ±0.005
 ANGLES ±1 DEGREE SURFACE FINISH 128 microinch RMS